




Metal liner insertion

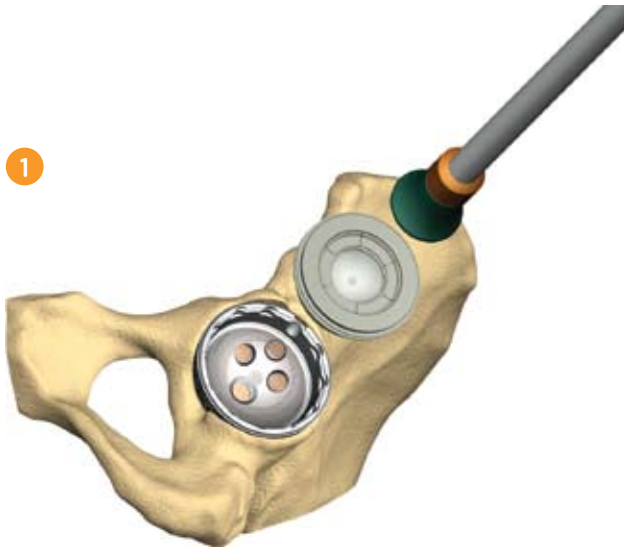


1 After the shell is implanted into the acetabulum, the surgeon inserts the liner with the attached alignment guide into the shell.

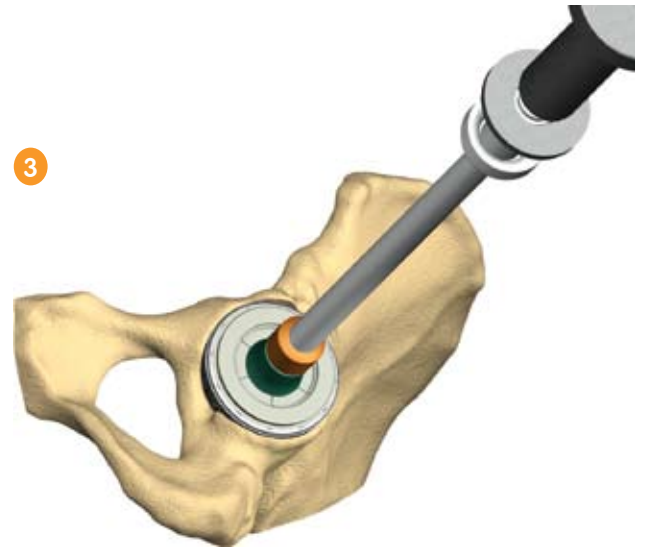

3 The surgeon then impacts the liner into the shell.

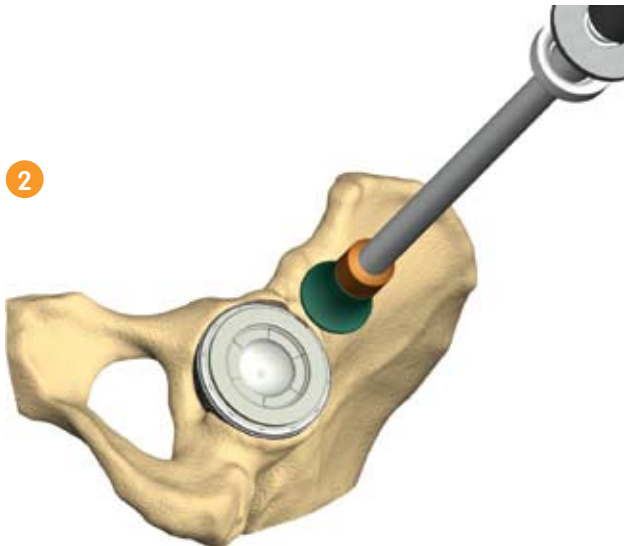

2 The cup impactor with impactor head is placed through the center of the alignment guide.

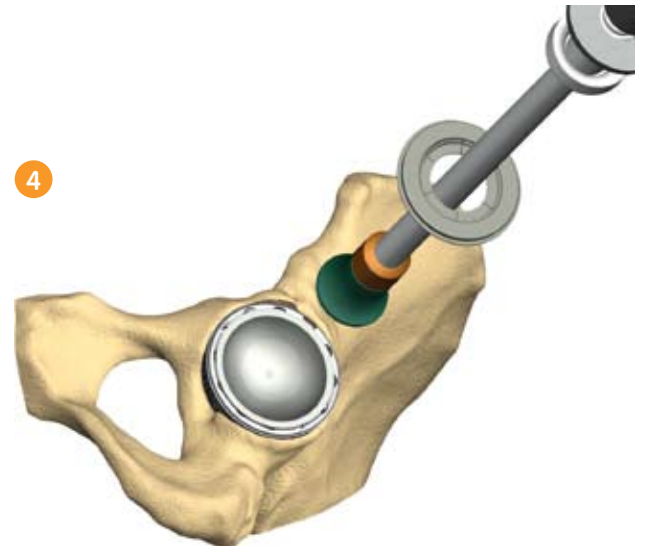

4 The alignment guide will disengage onto the shaft of the shell impactor and the liner will be perfectly seated inside the shell. The alignment guide can now be removed from the impactor for disposal.